


HPLC

Structure : Epithalon
Lot No : FMS201377-YY480474
Column : 4.6×250mm, YMC-Triart C18
Solvent A : 0.1% trifluoroacetic in 100% acetonitrile
Solvent B : 0.1% trifluoroacetic in 100% water
Gradient :
 A B
0.01min 10% 90%
25min 35% 65%
25.1min 100% 0%
30min STOP
Flow rate : 1.0 mL/min
Wavelength : 220nm
Volume : 5ul



Peak No.	Ret Time	Height	Area	Conc. .
1	9.285	367.297	3207.305	0.1645
2	10.313	532.119	9671.805	0.4959
3	10.770	170230.375	1932719.250	99.0993
4	11.530	345.759	3158.376	0.1619
5	12.352	237.900	1527.814	0.0783
Total			100.0000	

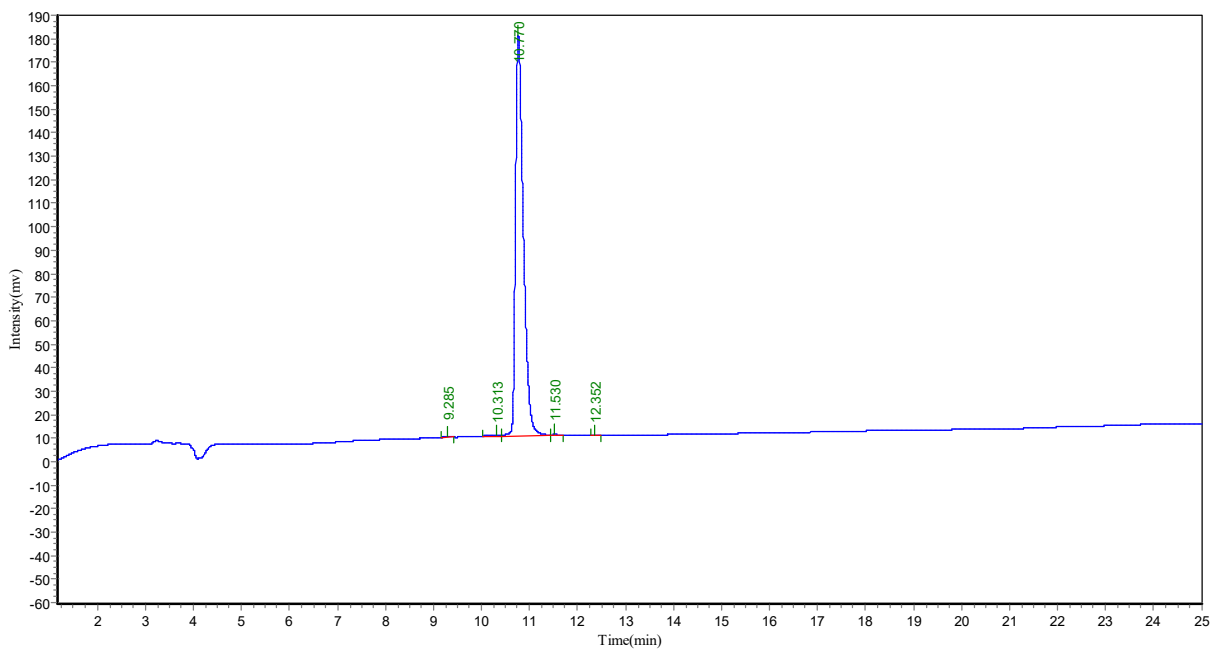